



EUROPattern

Computer-aided immunofluorescence microscopy (CAIFM)



- ✓ Fully automated microscopy and modern diagnostics at the computer screen (cell substrates, tissues and EUROPLUS antigen dots, also in mosaics)
- ✓ Pattern recognition for ANA, ANCA, AMA, anti-LKM (LKM-like) and mixed patterns based on deep convolutional neural networks, and calculation of titers
- ✓ Classification of results as positive or negative for *Crithidia luciliae*, antigen-expressing cells and EUROPLUS antigen dots
- ✓ Fast processing (13 seconds per image) and consolidation of results per patient for paperless diagnostics
- ✓ Digital archiving of fluorescence images and reports
- ✓ Bidirectional data exchange with the laboratory information system (LIS)



Modern technology from the experts

Magazine for 500 fields (A)

Automated slide supply

DataMatrix code reader

Controlled (c)LED for >50,000h constant light intensity (B)

High-resolution cameras


Precise optical system

Up to 3 different autofocus objectives

3D manual control


RealDrive manual control (C) (optional)

Oculars (optional)



Paperless generation of result reports in three steps

User-friendly software


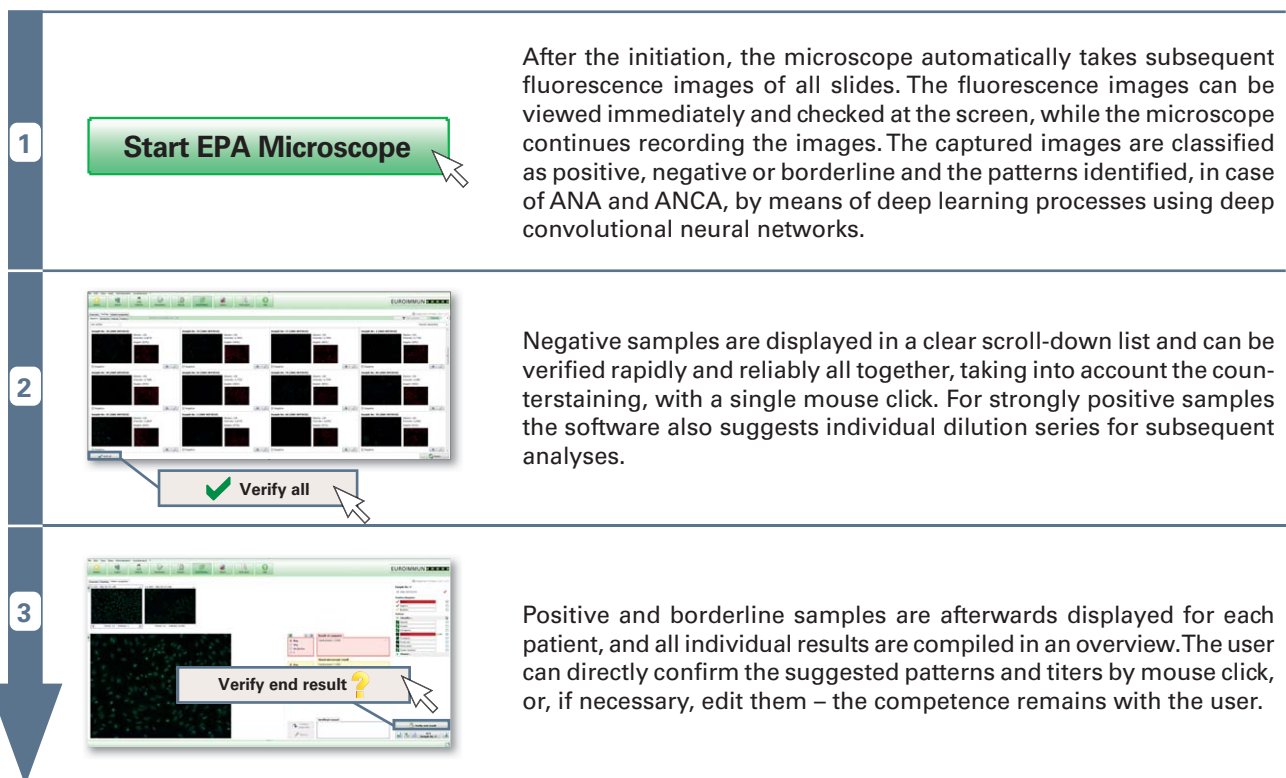


The entire process can be performed completely paperlessly, from the creation of worklists, to diagnostics and archiving of fluorescence images and results. Results from former analyses are shown in a clear patient history.




More practice-oriented functionalities

- ✓ The intelligent management of all data and results as well as the bi-directional communication with the LIS and the instruments takes place with the laboratory management software EUROLabOffice.
- ✓ Very quick focussing, image recording and digital evaluation (13 seconds/image) allow for the system to be integrated into the workflows of the largest laboratories. Diagnosis suggestions can be already verified during the automated microscopy process.
- ✓ Via mouse click (A), the sample field can be automatically approached and manually microscopied in the live mode. In order to prevent fading of the fluorescence, the cLED turns itself off when inactive.
- ✓ Automated photographing of tissues for subsequent visual diagnostics at the screen and archiving is also possible.
- ✓ By using the EUROLabOffice Image Atlas (B), recorded fluorescence images can be annotated and saved as a reference or for study purposes by one mouse click.

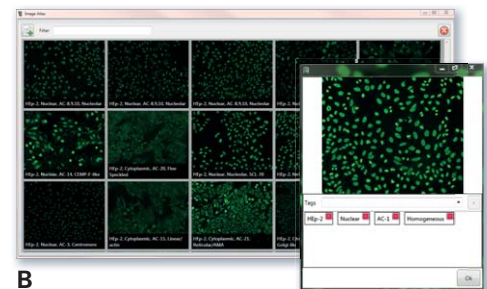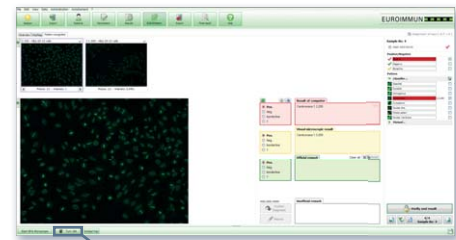

Fluorescence standardisation

- ✓ Constant illumination due to the built-in fluorescence standard
- ✓ Unique automated calibration of the microscope

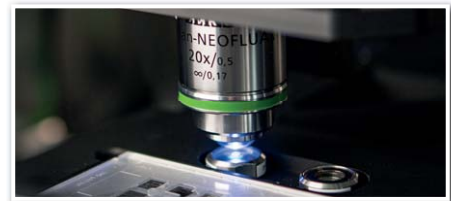

Excellent agreement between CAIFM and conventional evaluation

- ✓ Allocation of the samples to the corresponding results is ensured through the DataMatrix codes of the slides. The slides can be loaded in any order.
- ✓ Focussing in transmitted light prevents the fluorescence from fading.
- ✓ The counterstaining enables a reliable quality control of all fluorescence images during diagnostics.
- ✓ The controlled EUROIMMUN cLED guarantees standardised excitation light and reproducible fluorescence emissions.
- ✓ The integrated fluorescence standard calibrates all EUROPattern microscopes for comparable IIFT images.
- ✓ The computer-aided evaluation can be adjusted to the local diagnostic standards with respect to the patterns (e.g. sensitivity).
- ✓ Reliable support, both technical and scientific, is ensured. In the case of unclear findings, the user can automatically provide the EUROIMMUN support team with all required data in anonymised form for quick and targeted support.

ANA pattern	Identified pattern (automatic pattern recognition)	
	n	n %
Homogen.	15	14 93.3
Granular	12	11 91.7
Nucleolar	11	11 100
Centromeres	10	10 100
Nuclear dots	10	9 90
Cytoplasmic	22	22 100
DFS	20	100 100
Nucl. membr.	13	13 100
ANA neg.	79	75 94.9
Total	192	185 96.4

EUROPattern n = 171	Visual evaluation	
	Positive	Negative
Positive	92	4
Negative	0	75
Agreement	97.7%	
κ value	0.95	
Sensitivity	100%	
Specificity	94.9%	
Pos. prediction value	95.8%	
Neg. prediction value	100%	



Computer-aided evaluation of IIFT results using EUROPattern Pattern recognition based on deep convolutional neural networks


EUROPattern automatically generates result suggestions, including titer calculations, for a continually increasing number of substrates. This initially involves classification of the detected fluorescence patterns by means of deep convolutional neural networks, a deep-learning method. Finally, all the individual findings obtained with the substrates and dilutions are consolidated into a final result for each patient.

ANA diagnostics

- HEp-2/HEp-20-10 cells: Automatically generated pattern and titer suggestions with confidence values for nine fluorescence patterns according to ICAP* (homogeneous, speckled, dense fine-speckled, nucleolar, nuclear dots, centromeres, nuclear membrane, AMA and cytoplasmic) and any combinations thereof


*International Consensus on Antinuclear Antibody (ANA) Pattern

- *Critidia luciliae*: Automated positive–negative classification and titer suggestions based on the specific kinetoplast fluorescence for the detection of anti-dsDNA antibodies




ANCA diagnostics

- Granulocytes: Automatically generated pattern and titer suggestions with confidence values for the fluorescence patterns pANCA, cANCA and atypical ANCA
- EUROPLUS antigen dots: Automated positive–negative classification of the monospecific antigen fluorescence for confirmation and for differentiation from other diseases




Diagnostics based on antigen-expressing cells

- Neurology: Automated positive–negative classification and titer suggestions with confidence values for different antigens, e.g. AMPA 1/2, NMDAR, GABAR B1/B2, LGI1, CASPR2, DPPX, aquaporin-4 and MOG
- Nephrology: Automated positive–negative classification and titer suggestions with confidence values for the antigen PLA2R
- Infection diagnostics: Automated positive–negative classification and titer suggestions with confidence values for the antigens EBV-CA, EBV-EA and EBNA-1



Diagnostics of autoimmune liver diseases

- Liver (rat): Automated positive–negative classification for relevant ANA and identification of anti-LKM-like patterns ("LKM-like", is given as "anti-LKM" pattern after a confirmatory result on kidney tissue) to support the diagnosis of autoimmune hepatitis types 1 and 2
- Kidney (rat): Automated positive–negative classification for AMA, specific for primary biliary cholangitis, and identification of anti-LKM-like patterns ("LKM-like", is given as "anti-LKM" pattern after a confirmatory result on liver tissue; suspected autoimmune hepatitis type 2)



Scope of delivery

- EUROPattern microscope (incl. cameras, cLED, DataMatrix code reader, 20x objective, 3D manual control)
 - Optional: oculars, 10x objective, 40x objective, RealDrive manual control
- Magazine and carrier for automated slide loading (500 fields)
- PC system incl. control software for the EUROPattern microscope, high-resolution screen
- EUROPattern pattern recognition and result input software
- EUROLabOffice

Technical data

- Breadth x depth x height: approx. 51 cm x 66 cm x 85 cm
- Weight: approx. 82 kg
- Power supply: 110–240 V, 60 W, 50/60 Hz
- cLED light source for transmission light fluorescence microscopy
 - Constant excitation light source (460–490 nm)
- LED light source for transmitted light focussing
 - Constant light source (620–630 nm)

Subject to changes